

# HCal Timing Calibration Quality Checks

GMn, Config: 7, Prior to Pass 2

Sebastian SEEDS\*

June 25, 2024

## Contents

<b>1</b>	<b>How to Read this Document</b>	<b>1</b>
<b>2</b>	<b>Special Considerations</b>	<b>2</b>
<b>3</b>	<b>Timing</b>	<b>3</b>
3.a	ADC Time Offsets . . . . .	3
3.b	TDC Offsets . . . . .	5
3.c	ADC Time Aggregate Comparison . . . . .	8
<b>4</b>	<b>Time vs Run</b>	<b>9</b>
4.a	ADCt vs Run . . . . .	9
4.b	TDC vs Run . . . . .	10
<b>5</b>	<b>Supplemental Timing</b>	<b>12</b>
5.a	TDC Timewalk, Fits to Data . . . . .	12
5.b	ADCt Timewalk, Fit to Data . . . . .	14
<b>6</b>	<b>SBS-offline check</b>	<b>15</b>
6.a	ADC Time All Channels . . . . .	15
6.b	TDC All Channels . . . . .	16
<b>7</b>	<b>Supplemental</b>	<b>16</b>

## 1 How to Read this Document

This document details the timing calibration results for the above experiment, configuration, and replay pass. For information regarding the calibration process, see the [overleaf](#).

Each kinematic has been calibrated separately for timing and the database will reflect this moving forward. All time vs energy plots used for this calibration are generated using updated ADC gain parameters and timing offsets for accuracy.

---

\*email: sseeds@jlab.org

Each of the sections contains a brief description of the calibration results that follow. Any and all questions/concerns regarding these plots should be directed to the author at the email provided.

## 2 Special Considerations

- Evaluation of various timewalk fits are presented here as a preliminary assessment of a new timewalk calibration added to SBS-offline. Changes to SBS-offline to add this timewalk calibration are commensurate with this calibration. It is recommended that future passes consider a  $\Delta t = \alpha + \beta/E^N$  timewalk fit to the data where N is constrained to be very close to 0.5.

### 3 Timing

#### 3.a ADC Time Offsets

- Fits to ADC time spectra, by HCal Channel.

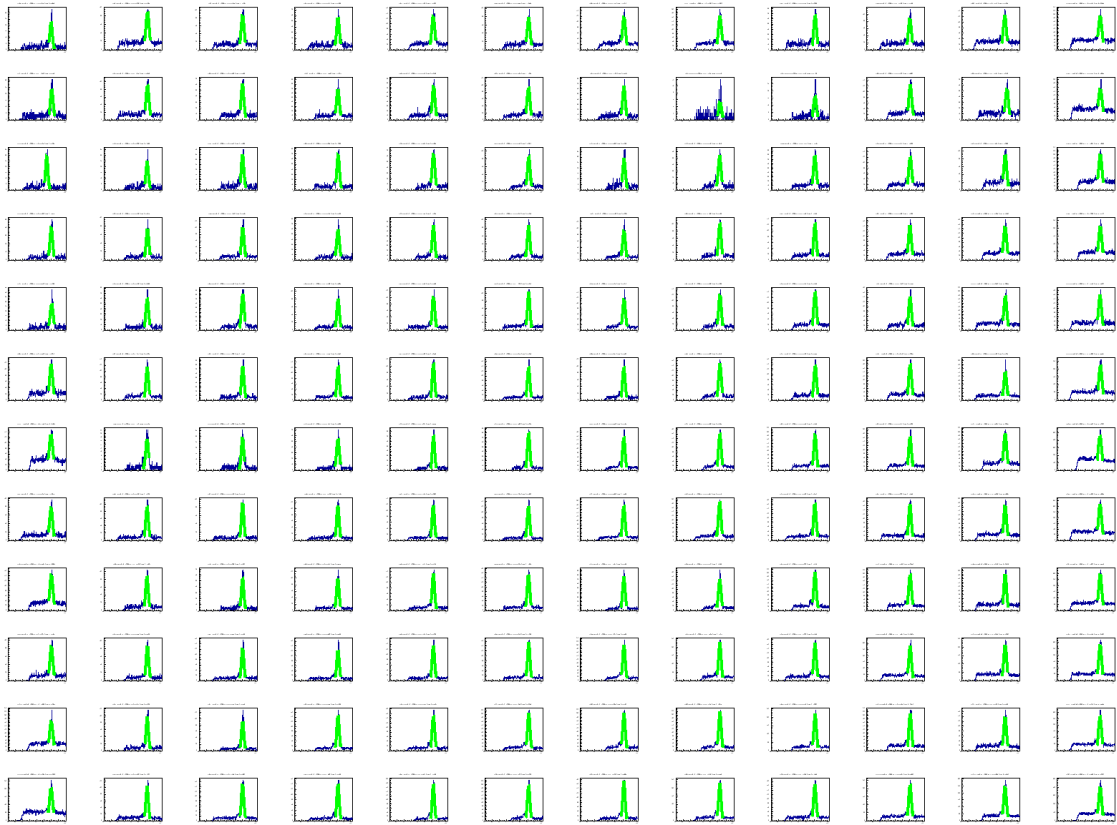


Figure 1: ADCt Spectra Fits vs. Channel, Top Half

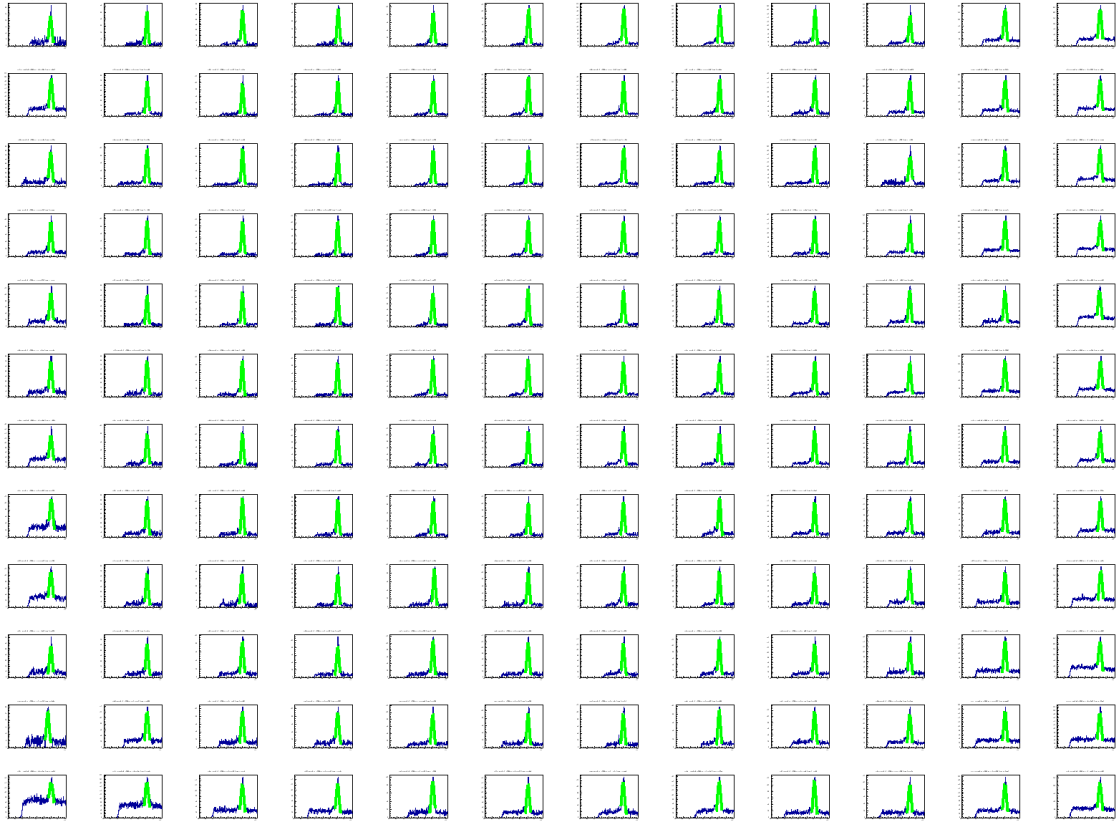


Figure 2: ADCt Spectra Fits vs. Channel, Bottom Half

- Mean/std. dev. comparisons before/after calibrations.

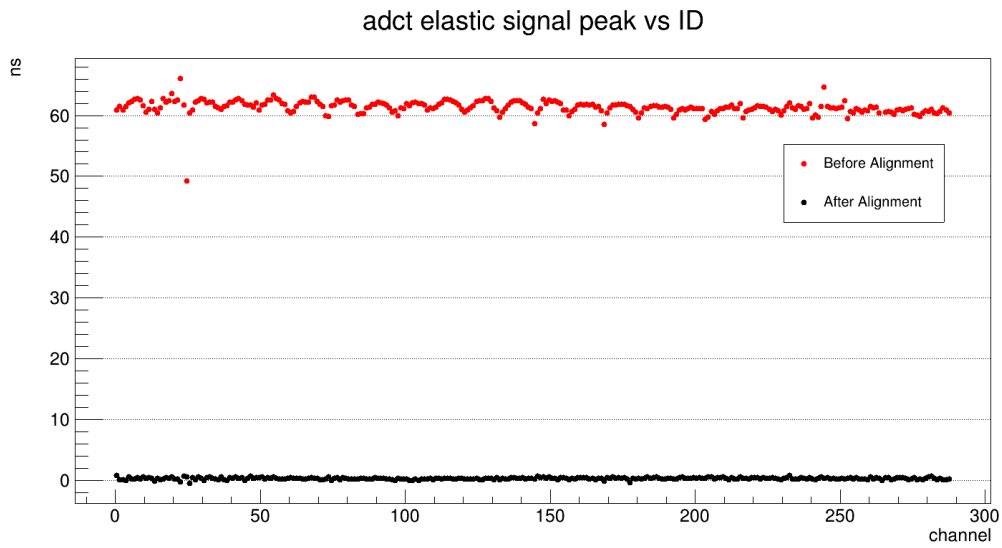


Figure 3: ADCt Fit Comparison, Post-Cal in Black

### 3.b TDC Offsets

- Fits to TDC spectra, by HCal Channel.

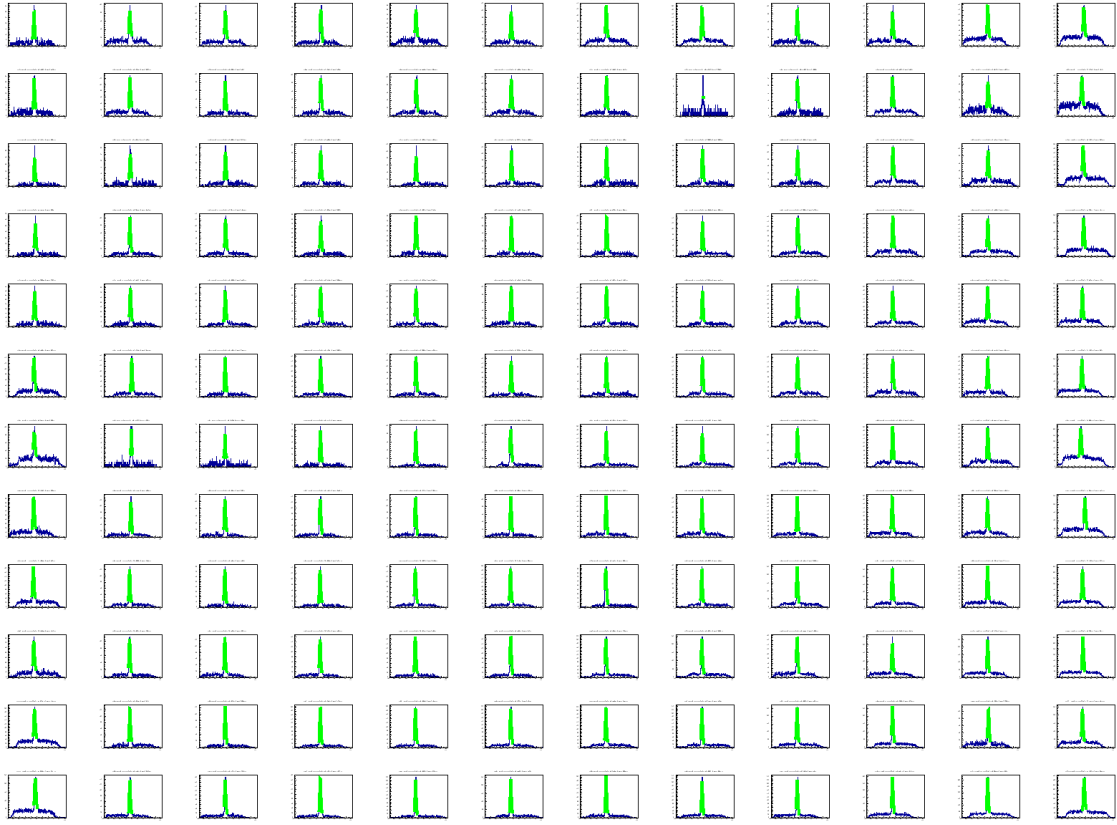


Figure 4: TDC Spectra Fits vs. Channel, Top Half

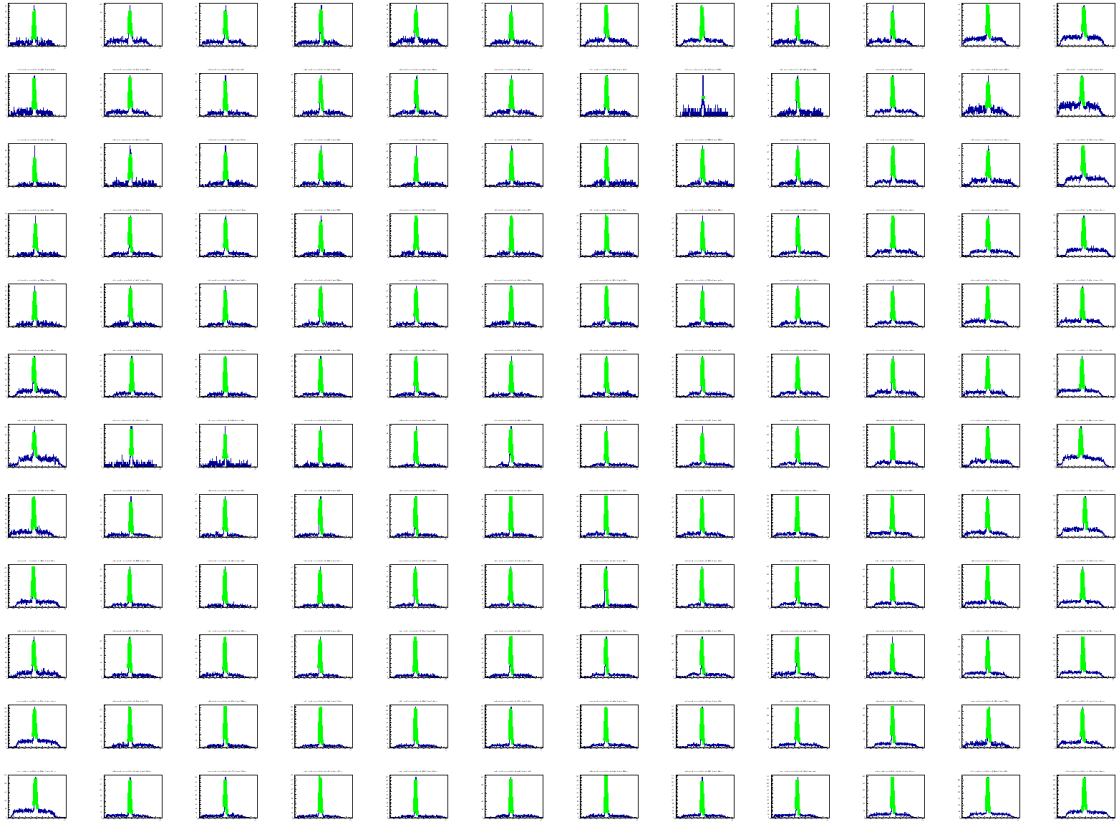


Figure 5: TDC Spectra Fits vs. Channel, Bottom Half

- Mean/std. dev. comparisons before/after calibrations.

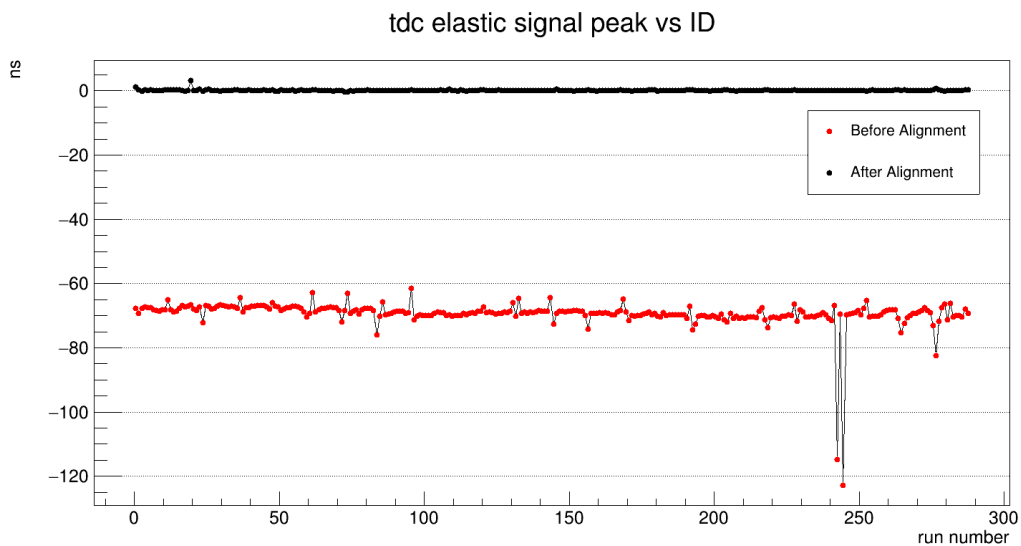


Figure 6: TDC Fit Comparison, Post-Cal in Black

### 3.c ADC Time Aggregate Comparison

All blocks post-alignment ADC time fit and comparison with ADC time from data before per-channel alignment.

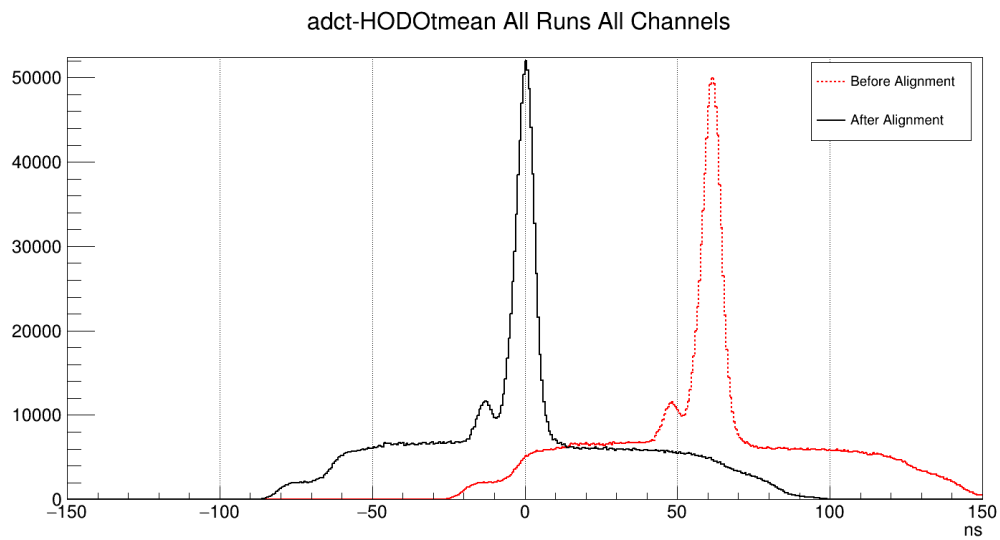


Figure 7: ADCt Comparison, All Channels. Post-alignment Mean: **0.19 ns**



## 4 Time vs Run

No significant deviations occur on either ADCt or TDC data as a function of run number.

### 4.a ADCt vs Run

HCal adc time (all blocks) vs run number, before and after. Includes direct comparison.

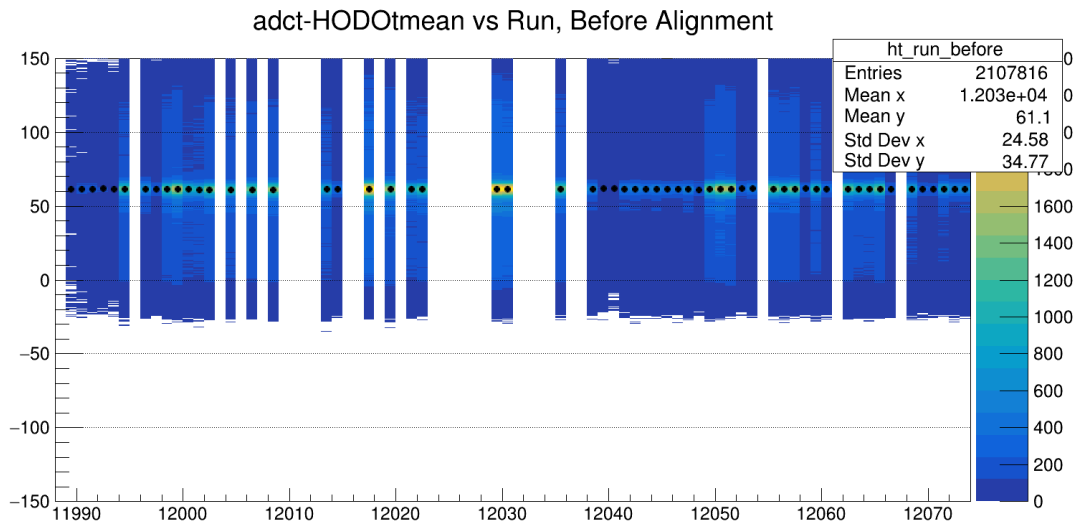


Figure 8: HCal ADCt vs Run Number All Channels, Before Alignment

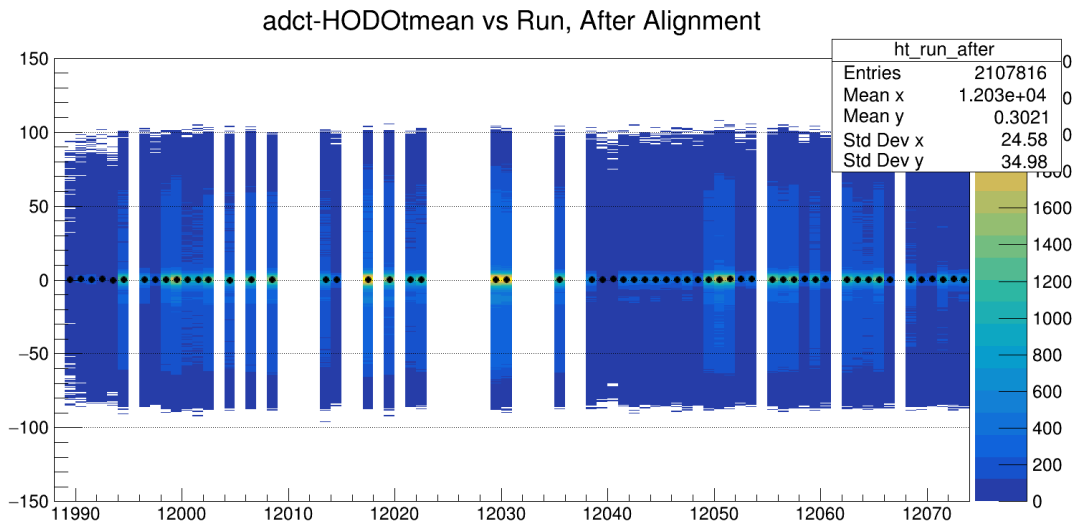


Figure 9: HCal ADCT vs Run Number All Channels, After Alignment

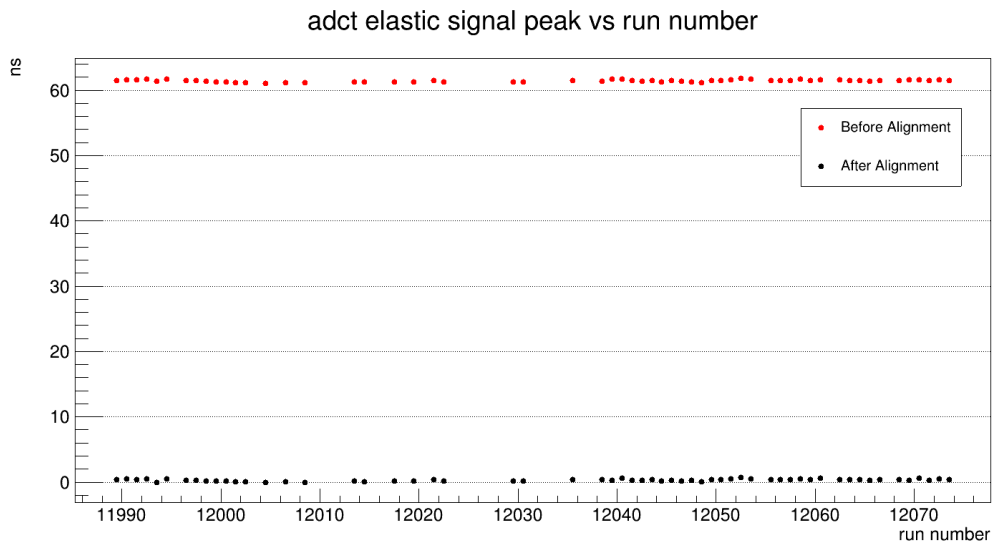


Figure 10: HCal ADCT vs Run Number All Channels, Comparison

#### 4.b TDC vs Run

HCal tdc time (all blocks) vs run number, before and after. Includes direct comparison.

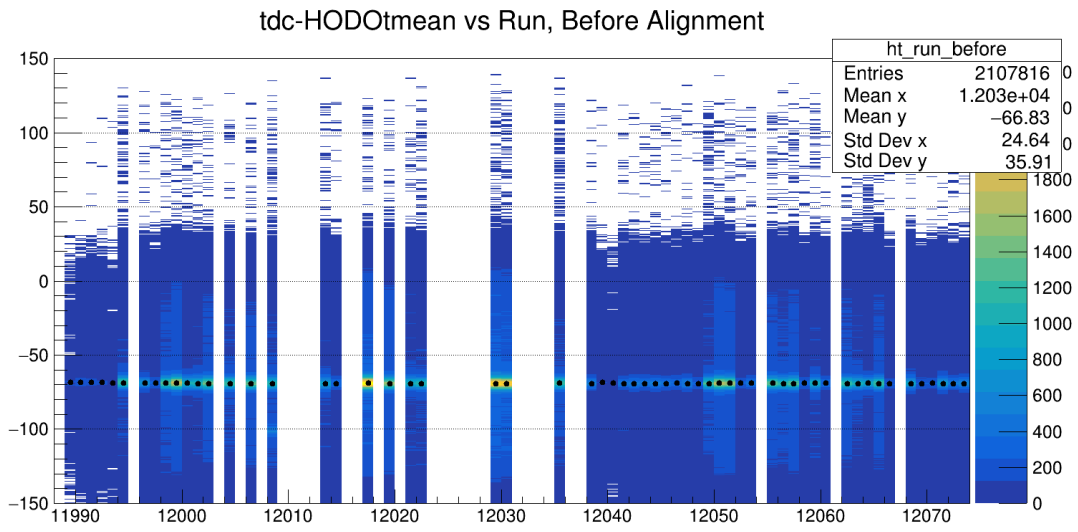


Figure 11: HCal TDC vs Run Number All Channels, Before Alignment

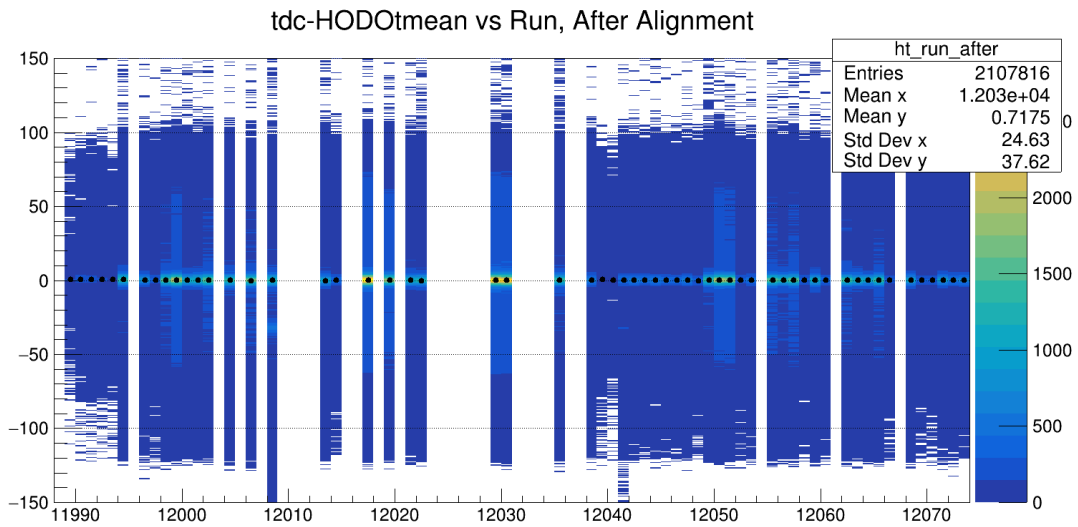


Figure 12: HCal TDC vs Run Number All Channels, After Alignment

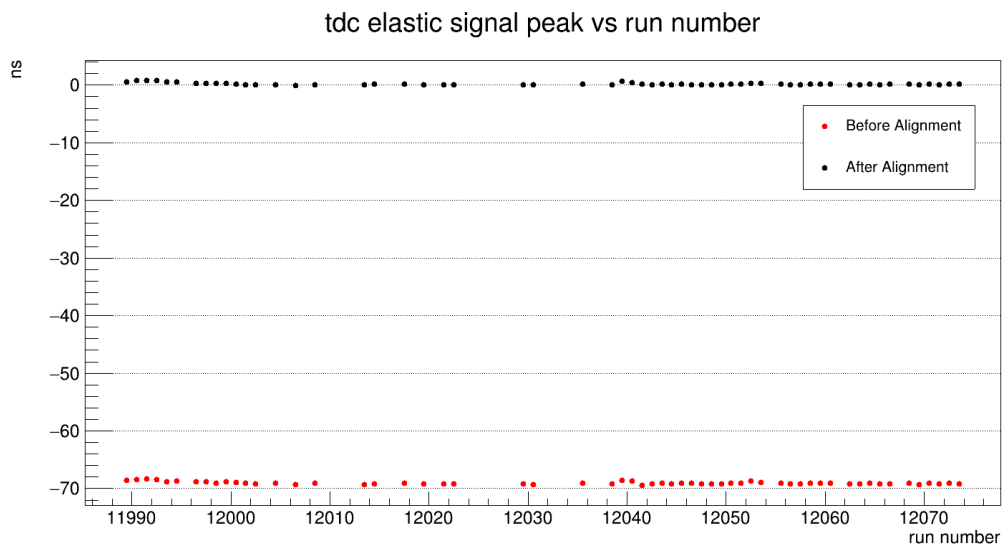


Figure 13: HCal TDC vs Run Number All Channels, Comparison

## 5 Supplemental Timing

### 5.a TDC Timewalk, Fits to Data

HCal tdc time (all blocks) vs energy, fit with  $\Delta t = p_0 + p_1 \cdot E$ .  $p_0$  is normal to the data and not passed to the calibration.

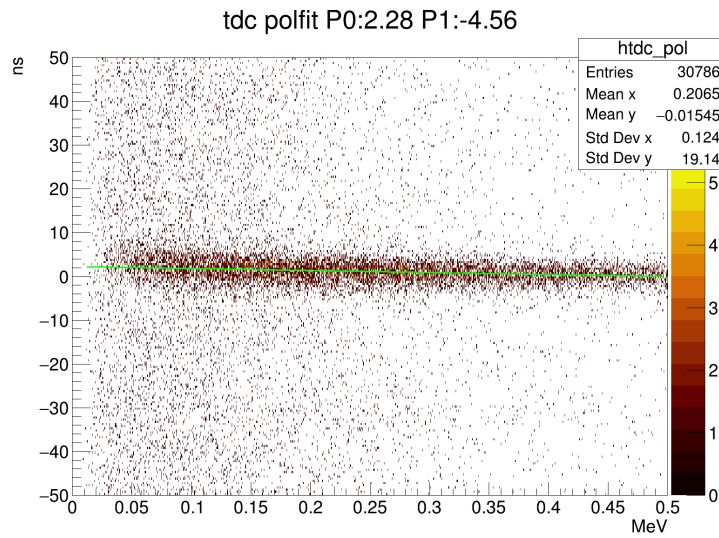


Figure 14: HCal TDC vs E

HCal tdc time (all blocks) vs energy, fit with  $\Delta t = P0 \cdot \exp(-P1 \cdot E) + p2$ .  $p2$  is normal to the data and not passed to the calibration.

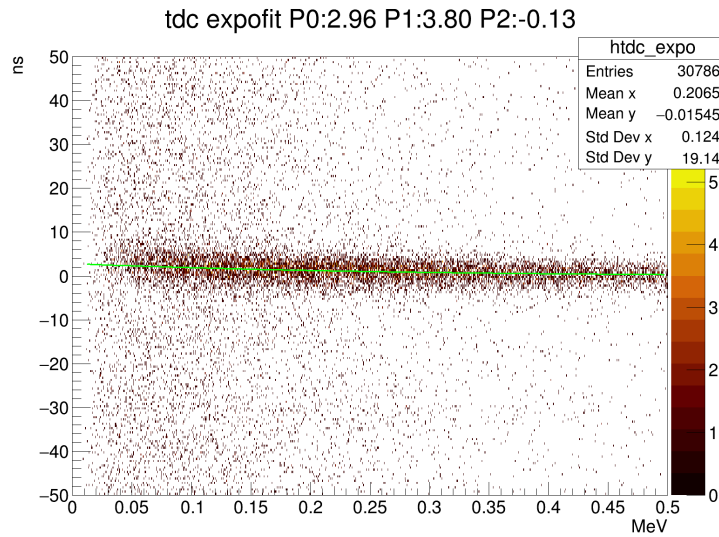


Figure 15: HCal TDC vs E

HCal tdc time (all blocks) vs energy, fit with  $\Delta t = p0 + p1/E^{p2}$ .  $p0$  is normal to the data and not passed to the calibration.

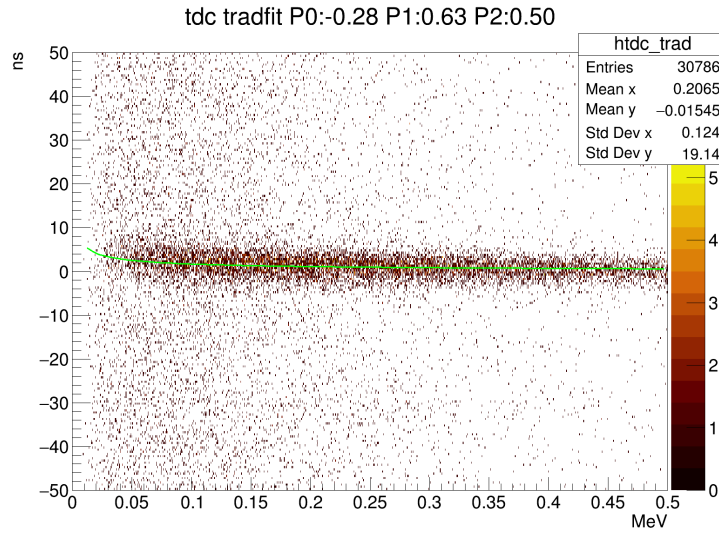


Figure 16: HCal TDC vs E,

### 5.b ADCt Timewalk, Fit to Data

HCal adct time (all blocks) vs energy, fit with  $\Delta t = p_0 + p_1 \cdot E$ .  $p_0$  is normal to the data and not passed to the calibration.

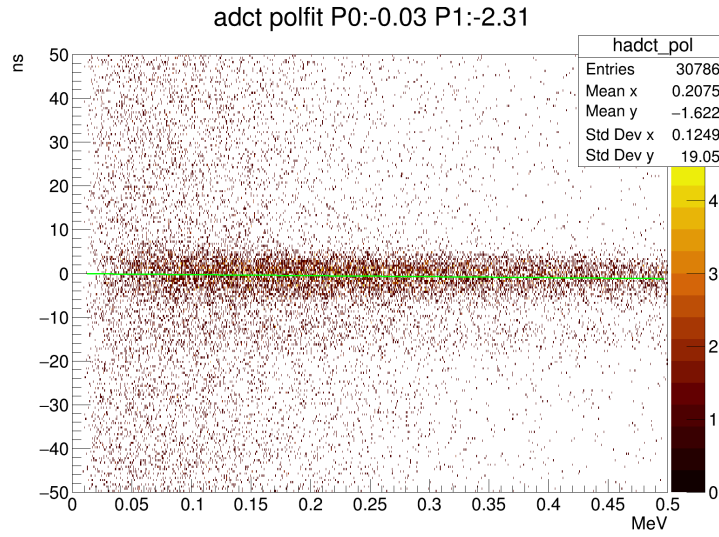


Figure 17: HCal ADCt vs E

## 6 SBS-offline check

The following plots repeat checks above, but with a small replay of run 12049 data using `replay_gmn.C` with SBS-offline associated libraries updated with timewalk and with new offsets included in the database

### 6.a ADC Time All Channels

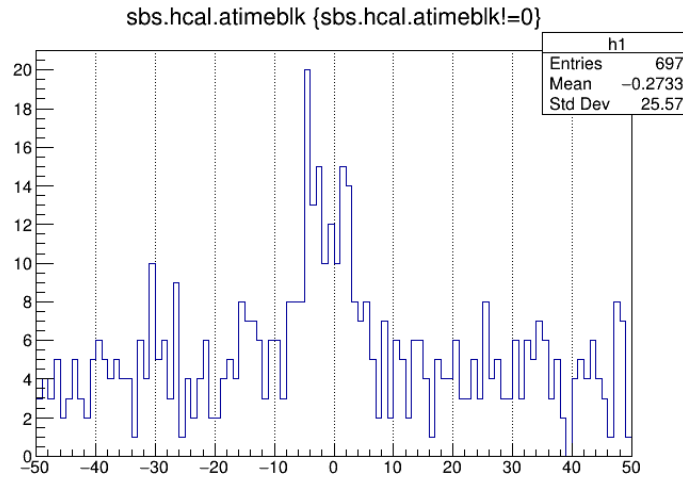


Figure 18: ADCt All Channels, Run 12049

## 6.b TDC All Channels

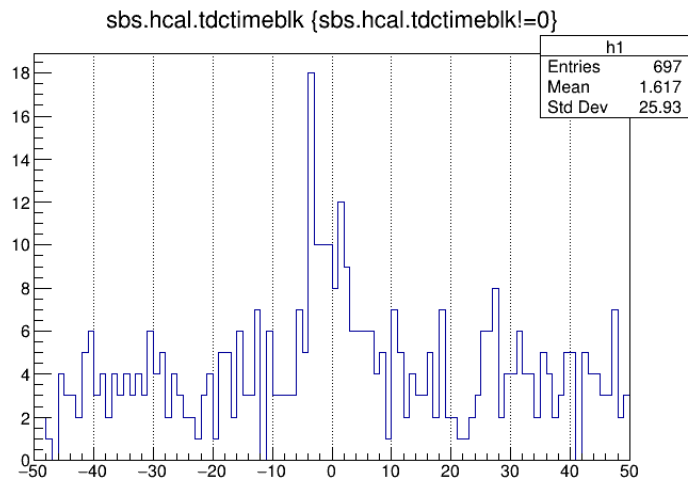


Figure 19: TDC All Channels, Run 12049

## 7 Supplemental

General Set ADCT Alignment Info  
Experiment: gmn, Configuration: 7, Pass: 0  
Creation Date: 9\_14\_2023  
Run range 0 - 0  
Exclusion range 0 - 0  
Target(s) Used: All Available  
Calibration Set: none

Elastic Cuts  
Global Elastic Cuts:  $bb.tr.n > 0 \& \& abs(bb.tr.vz[0]) < 0.08 \& \& bb.gem.track.nhits > 2 \& \& bb.tr.p[0] > 2.0 \& \& sbs.hcal.e > 0.03 \& \& bb.ps.e > 0.2$

Other Cuts  
Minimum Ev per Cell : 50  
HCal Acceptance Match (Projected Nucleon Within HCal Acceptance)

Figure 20: SBS7 adct timing cuts and experimental parameters.



General Set TDC Alignment Info

Experiment: gmn, Configuration: 7, Pass: 0

Creation Date: 9\_14\_2023

Run range 0 - 0

Exclusion range 0 - 0

Target(s) Used: All Available

Calibration Set: none

Elastic Cuts

Global Elastic Cuts:  $bb.tr.n=0 \& \& abs(bb.tr.vz[0]) < 0.08 \& \& bb.gem.track.nhits > 2 \& \& bb.tr.p[0] > 2.0 \& \& sbs.hcal.e > 0.03 \& \& bb.ps.e > 0.2$

Other Cuts

Minimum Ev per Cell : 50

HCal Acceptance Match (Projected Nucleon Within HCal Acceptance)

Figure 21: SBS7 tdc timing cuts and experimental parameters.